


UniSeal®

ProDerma®
Powder-Free

Smooth or Textured
Latex Exam Gloves

**S
P
E
C
S**



Sizes:	Item #:	
	Smooth:	Textured:
XS	010-5	011-5
S	010-6	011-6
M	010-7	011-7
L	010-8	011-8
XL	010-9	011-9

9"
cuff

5
mil



ISO
9002

Quality Standards:

- Meets or exceeds the following standards: ASTM D3578-01ae2 (USA), EN 455 (EEC), AS 40 (Australia), FDA, CE
- Quality sampled in accordance with MIL.STD 105D
- ISO 9002 Certified Manufacturing
- Meets the Viral Penetration Test (ASTM F1671-03)



Type: **Non-Sterile Examination Glove**
Shape: **Ambidextrous**

Manufacturing Standards

Brand new state-of-the-art manufacturing plant with computer-controlled market-leading technology.

Defect	Inspection Level	AQL
Pinholes (FDA 1000ml watertight test)	Level 11	1.5
Visual Defects (major)	S-4	1.5
Visual Defects (minor)	S-4	2.5
Dimensions	S-2	4.0

Physical Properties

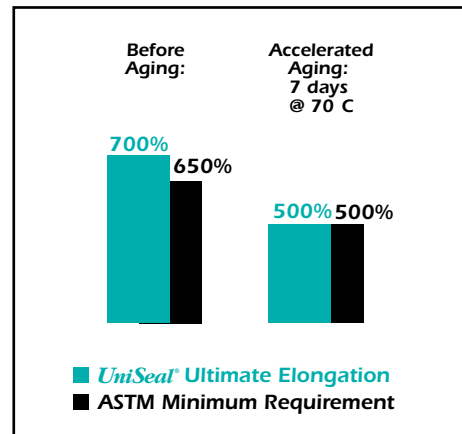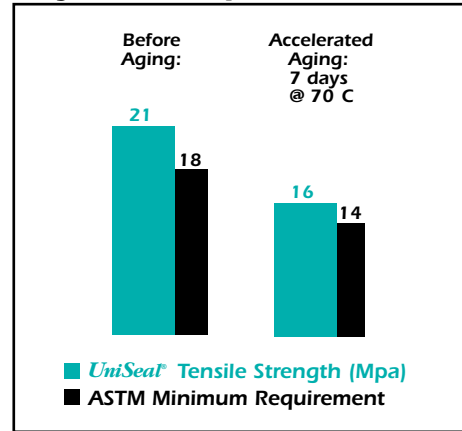

Dimensions (all measurements in mm)

Glove Length	Palm Width ±10mm	THICKNESS		
		Cuff	Palm	Finger
240	75	0.14	0.16	0.18
245	85	0.14	0.16	0.18
245	95	0.14	0.16	0.18
245	105	0.14	0.16	0.18
245	115	0.14	0.16	0.18