

UniSeal®

High-Risk

Powder-Free



Textured Latex Exam Gloves

Manufacturing Standards


Brand new state-of-the-art manufacturing plant with computer-controlled market-leading technology.

Defect	Inspection Level	AQL
Pinholes (FDA 1000ml watertight test)	Level 11	1.5
Visual Defects (major)	S-4	1.5
Visual Defects (minor)	S-4	2.5
Dimensions	S-2	4.0

Physical Properties

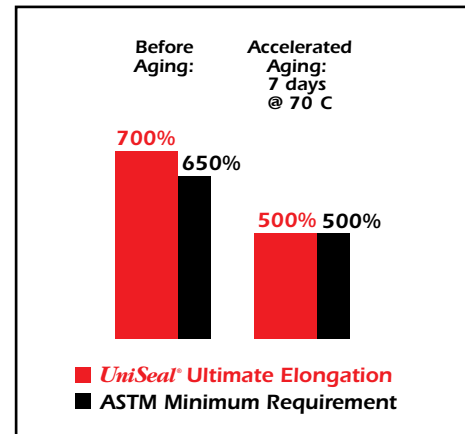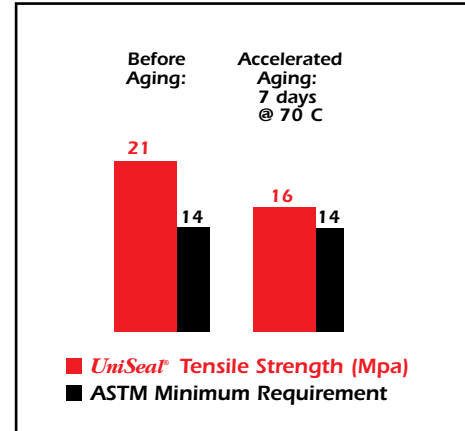

S
P
E
C
S



Item #:	
Sizes:	Textured:
S	015-6
M	015-7
L	015-8
XL	015-9
XXL	015-0

12" cuff
15 mil

ISO 9001:2000

THIS GLOVE MEETS THE EMERGENCY MEDICAL EXAMINATION GLOVE REQUIREMENTS OF NFPA 1999, STANDARD ON PROTECTIVE CLOTHING FOR EMERGENCY MEDICAL OPERATIONS, 2003 EDITION. THIS GLOVE IS FOR SINGLE USE ONLY.

IN ACCORDANCE WITH NFPA 1999(2003) 38DF

Quality Standards:

- Meets or exceeds the following standards: ASTM D3578-01ae2 (USA), EN 455 (EEC), AS 40 (Australia), FDA, CE
- Quality sampled in accordance with MIL-STD 105D
- ISO 9001:2000 and GMP
- Meets the Viral Penetration Test (ASTM F1671-03)

Allergen/Contact Sensitizer Exclusion
(Powder-Free): Butylhydroxyanisole (BHA); 3, 5 Di-tertiary butyl 4-hydroxytoluene (BHT); Mercaptobenzothiazole (MBT); Amine antioxidant derivatives (IPPD, CPPD, DPPD) or any other chemicals of the PPD mix; Zinc diethyldithiocarbamate (ZDEC) and Zinc dibutyldithiocarbamate (ZDBC) or any other chemicals of the carbamate group; Tetramethylthiuram disulfide (TMTD); 4.4 Thiobis (6-Tertiary Butyl) Meta cresol.

Dimensions (all measurements in mm)

Glove Length	Palm Width +/- 3 mm	THICKNESS +/- 3 mm		
		Cuff	Palm	Finger
(XS)300	76	0.12	0.15	0.19
(S) 300	84	0.12	0.15	0.19
(M) 300	94	0.12	0.15	0.19
(L) 300	105	0.12	0.15	0.19
(XL)300	111	0.12	0.15	0.19

Type: Non-Sterile Examination Glove

Shape: Ambidextrous