

# UniSeal®

## Sur-G-Glove® Lightly Powdered


**Textured  
Sterile Latex Exam Gloves**

### Manufacturing Standards

Brand new state-of-the-art manufacturing plant with computer-controlled market-leading technology.

Defect	Inspection Level	AQL
Pinholes (FDA 1000ml watertight test)	Level 11	1.5
Visual Defects (major)	S-4	1.5
Visual Defects (minor)	S-4	2.5
Dimensions	S-2	4.0

**S  
P  
E  
C  
S**



Item #:



Sizes:	Sur-G-Glove®	Sensiflex®
5½	025-5.5	030-5.5
6	025-6.0	030-6.0
6½	025-6.5	030-6.5
7	025-7.0	030-7.0
7½	025-7.5	030-7.5
8	025-8.0	030-8.0
8½	025-8.5	030-8.5
9	025-9.0	030-9.0

**12"**  
cuff

**5**  
mil

**ISO  
9002**

### Physical Properties

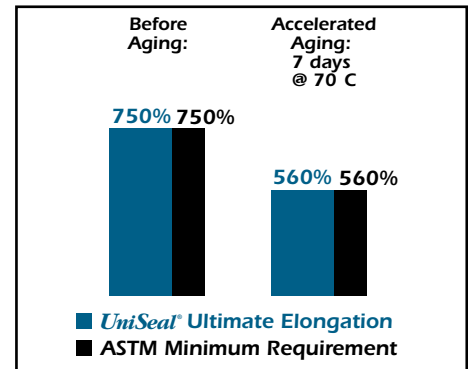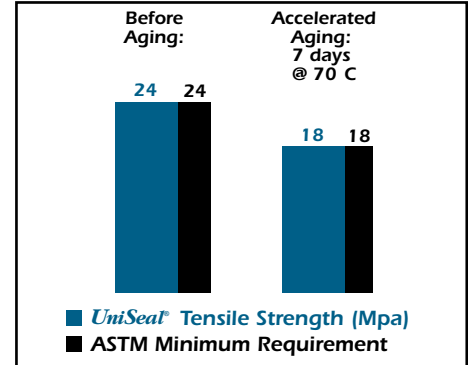

### Quality Standards:

- Meets or exceeds the following standards:  
ASTM D3577-00, ASTM D6124-00 (USA), EN 455 (EEC), AS 40 (Australia), JIS T 9107, SABS 1155 FDA, CE
- Quality sampled in accordance with MIL.STD 105D
- ISO 9002 Certified Manufacturing
- Meets the Viral Penetration Test (ASTM F1671-03)\*
- Passes 200 Modified Human Draize Skin Allergy Test\*

**Allergen/Contact Sensitizer Exclusion**  
(Powder-Free): Butylhydroxyanisole (BHA); 3, 5 Di-tertiary butyl 4-hydroxytoluene (BHT); Mercaptobenzothiazole (MBT); Amine antioxidant derivatives (IPPD, CPPD, DPPD) or any other chemicals of the PPD mix; Zinc diethyldithiocarbamate (ZDEC) and Zinc dibutyldithiocarbamate (ZDBC) or any other chemicals of the carbamate group; Tetramethylthiuram disulfide (TMTD); 4,4 Thiobis (6-Tertiary Butyl) Meta cresol.

### Dimensions

(all measurements in mm)

Glove Length	Palm Width +/- 6mm	THICKNESS		
		Cuff	Palm	Finger
(5.5)300	71	0.10	0.13	0.17
(6.0)300	77	0.10	0.13	0.17
(6.5)300	83	0.10	0.13	0.17
(7.0)300	89	0.10	0.13	0.17
(7.5)300	95	0.10	0.13	0.17
(8.0)300	102	0.10	0.13	0.17
(8.5)300	108	0.10	0.13	0.17
(9.0)300	114	0.10	0.13	0.17

Type: Sterile Surgical Glove  
Shape: Anatomic

\*Sensiflex® only