

UniSeal®

SureGrip®
Powder-Free

**Textured, Low Protein
Latex Exam Gloves**

Manufacturing Standards

Brand new state-of-the-art manufacturing plant with computer-controlled market-leading technology.

Defect	Inspection Level	AQL
Pinholes (FDA 1000ml watertight test)	Level 11	1.5
Visual Defects (major)	S-4	1.5
Visual Defects (minor)	S-4	2.5
Dimensions	S-2	4.0

S




Sizes: Item #:

X Small	035-5
Small	035-6
Medium	035-7
Large	035-8
X Large	035-9

P



E



C



S



9"
cuff

5
mil



ISO
9002

Physical Properties

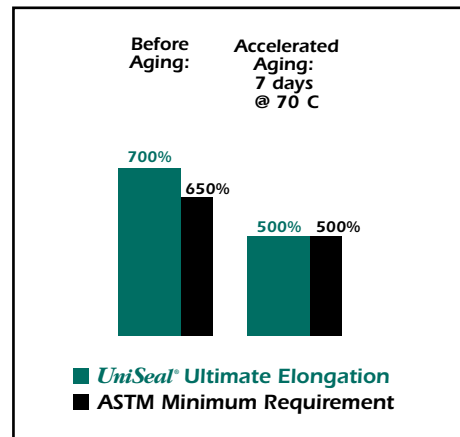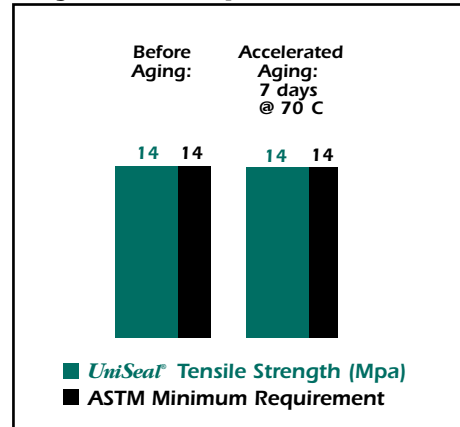

Quality Standards:

- Meets or exceeds the following standards: ASTM D3578-01 ea2 (USA), EN 455 (EEC), AS 40 (Australia), FDA, CE
- Quality sampled in accordance with MIL-STD 105D
- Passes the 200 Human Modified Draize Skin Allergy Test
- ISO 9002 Certified Manufacturing

Dimensions (all measurements in mm)

Glove Length	Palm Width +/-0.03mm	THICKNESS +/-0.03mm		
		Cuff	Palm	Finger
(XS) 240	76	0.12	0.15	0.19
(S) 240	84	0.12	0.15	0.19
(M) 240	94	0.12	0.15	0.19
(L) 240	105	0.12	0.15	0.19
(XL) 240	113	0.12	0.15	0.19

Type: Non-Sterile Examination Glove

Shape: Ambidextrous