


UniSeal®

Gold
Lightly Powdered
Latex Exam Gloves

S
P
E
C
S



Sizes: Item #:

X Small	080-5
Small	080-6
Medium	080-7
Large	080-8
X Large	080-9

9"
cuff

5
mil





ISO
9002

Manufacturing Standards

Brand new state-of-the-art manufacturing plant with computer-controlled market-leading technology.

Defect	Inspection Level	AQL
Pinholes (FDA 1000ml watertight test)	Level 11	1.5
Visual Defects (major)	S-4	1.5
Visual Defects (minor)	S-4	2.5
Dimensions	S-2	4.0

Physical Properties

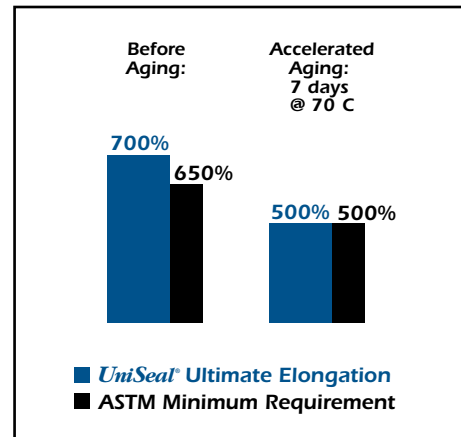

Quality Standards:

- Meets or exceeds the following standards: ASTM D3578-01ae2 (USA), EN 455 (EEC), AS 40 (Australia), FDA, CE
- Quality sampled in accordance with MIL.STD 105D
- ADA Accepted
- ISO 9002 Certified Manufacturing
- Powder: 100% U.S.P. surgical-grade Cornstarch

Type: Non-Sterile Examination Glove
Shape: Ambidextrous

Dimensions (all measurements in mm)

Glove Length	Palm Width ±/-.0.03mm	THICKNESS ±/-.0.03mm		
		Cuff	Palm	Finger
(XS) 240	76	0.12	0.15	0.16
(S) 240	84	0.12	0.15	0.16
(M) 240	94	0.12	0.15	0.16
(L) 240	105	0.12	0.15	0.16
(XL) 240	113	0.12	0.15	0.16