


UniSeal®

**Sterile Procedure
Powdered / Powder-Free**

Latex Procedure Gloves

**S
P
E
C
S**



Sizes:	Item #:	
	Pairs:	Pairs:
Small	142-6	242-6
Medium	142-7	242-7
Large	142-8	242-8
X-Large	142-9	242-9





ISO 9001:2000

Manufacturing Standards

Brand new state-of-the-art manufacturing plant with computer-controlled market-leading technology.

Defect	Inspection Level	AQL
Pinholes (FDA 1000ml watertight test)	Level 11	1.5
Visual Defects (major)	S-4	1.5
Visual Defects (minor)	S-4	2.5
Dimensions	S-2	4.0

Physical Properties

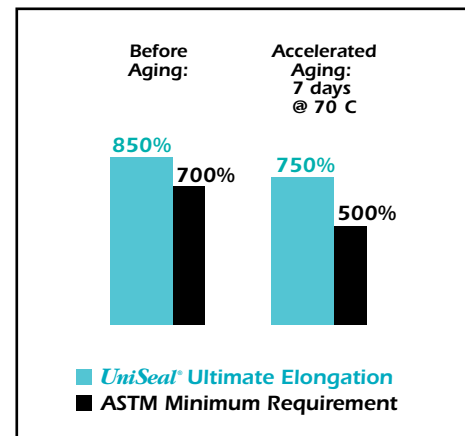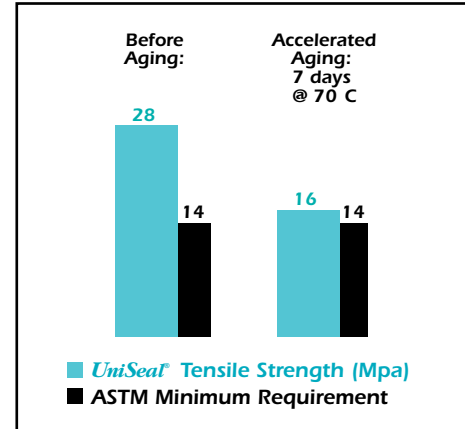

Quality Standards:

- Meets or exceeds the following standards: ASTM (USA), EN 455 (EEC), AS 40 (Australia), FDA, CE
- Quality sampled in accordance with MIL.STD 105D
- ISO 9001:2000 Certified Manufacturing

Allergen/Contact Sensitizer Exclusion
(Powder-Free): Butylhydroxyanisole (BHA); 3, 5 Di-tertiary butyl 4-hydroxytoluene (BHT); Mercaptobenzothiazole (MBT); Amine antioxidant derivatives (IPPD, CPPD, DPPD) or any other chemicals of the PPD mix; Zinc diethyldithiocarbamate (ZDEC) and Zinc dibutyldithiocarbamate (ZDBC) or any other chemicals of the carbamate group; Tetramethylthiuram disulfide (TMTD); 4,4 Thiobis (6-Tertiary Butyl) Meta cresol.

Dimensions (all measurements in mm)

Glove Length	Palm Width ±/10mm	THICKNESS		
		Cuff	Palm	Finger
240	85	0.14	0.16	0.18
240	95	0.14	0.16	0.18
240	105	0.14	0.16	0.18
240	105	0.14	0.16	0.18

Type: Sterile Latex Examination Glove

Shape: Ambidextrous